


LaserMount™

244

USER'S MANUAL

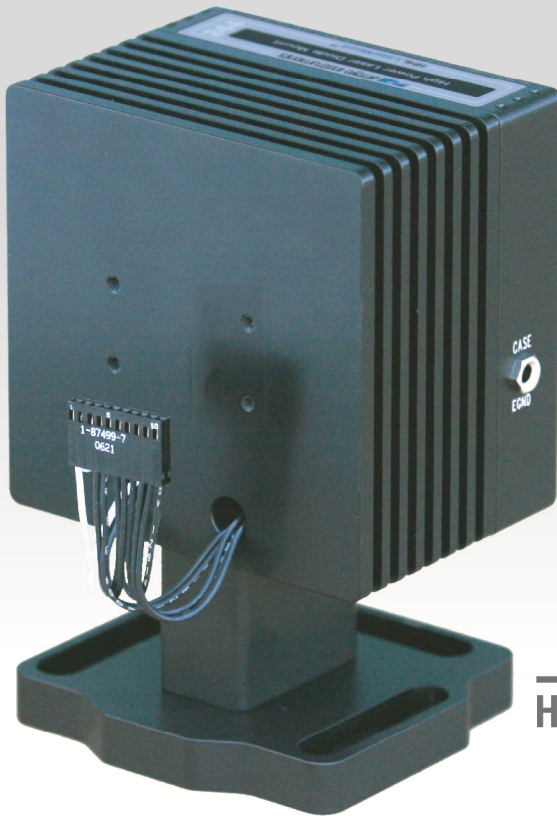

HHL MOUNT

Introduction

Thank you for choosing the **244 HHL LaserMount** from Arroyo Instruments. The **244 LaserMount** is designed for high performance and long term use.

For electrical connections, the **244 LaserMount** features a slide on connector that is pre-wired for HHL devices, making electrical connection to the HHL a snap. Simply load the HHL device into the fixture and slide on the connector.

The **244 LaserMount** comes standard with an integrated fan for additional cooling capacity. When used with the **5300 Series TECSource** temperature controllers, no additional power supply is needed to power the fan, or use a standard external 12V DC power supply when connecting to other temperature controllers.

The **244 LaserMount** also offers all the features you would expect from a modern HHL laser diode fixture, including:

- Designed to be quickly integrated with Arroyo's **LaserSource** and **TECSource** instruments.
- Industry-standard D-sub connectors and pin-outs allow for quick integration into existing laser applications.
- Banana plug for case ground, which can be used as a wrist strap connection or to assure proper grounding to an optical table or test bench.



Installation and Use

The **244 LaserMount** setup is very quick, simply follow the directions below.

Earth Grounding Considerations:

When using the **244 LaserMount** with Arroyo Instruments' **LaserSource** or **TECSource** and cables, the **244** will be earth grounded through the cables and instrument. However, if you are using another vendor's cables or instruments, verify the earth ground path and that proper grounding techniques are used. The mount has a banana jack that provides a case connection which can be used for a wrist strap (if the case is earth grounded) or to tie the case to earth ground through something other than the laser driver or temperature controller.

Internal Cooling Fan:

The **244 LaserMount** has an integrated cooling fan for the heat sink, which allows operation at high heat loads. If you are using an Arroyo Instruments **5300 Series TECSource** temperature controller, the fan supply is built directly into the **TECSource**. You will need to enable the fan supply in the **TECSource** menu – see the **TECSource** manual for additional details.

If you are using a third-party temperature controller, then you will need to provide a 12V DC power supply. The connection into the mount is a standard 2.1mm round plug with the center pin positive, and must be capable of supplying at least 150mA.

The fan +12VDC and ground connections are completely isolated from the rest of the fixture.

For quieter fan operation, the voltage can be reduced as low as 8VDC, although there will be a slight reduction in thermal capability due to the slower fan speed.

Connect to Laser Diode Driver and TEC Controller:

Connect the **244 LaserMount** to your laser diode driver and temperature controller. Where possible, we recommend the use of Arroyo Instruments laser and TEC cables. Use p/n 1260 **TECSource** Cable for the temperature controller connection, and p/n 1220 **LaserSource** Cable for the laser connection.

NOTE

Arroyo Instruments offers Laser and TEC cables designed to connect directly between our **LaserSource** and **TECSource** products. If you use your own cables, ensure the connections are properly made between the instrument and the mount, and that proper grounding techniques are used. The pin-out of the connectors can be found later in this document.

WARNING


Be sure you are properly ESD protected before handling your laser. For additional information, read the section titled "Laser Diode Protection" later in this manual.

Mounting your device:

Using the provided 6-32 screws, screw the device down to the mount using the four mounting holes on the face of the fixture. Tighten the screws sufficiently to provide good clamping force to the fixture, but do not over-tighten, as you may strip the threads.

For better thermal transfer, heat sink compound or a thermal pad may be used.

The drawing below illustrates how to load the device onto the **LaserMount**:

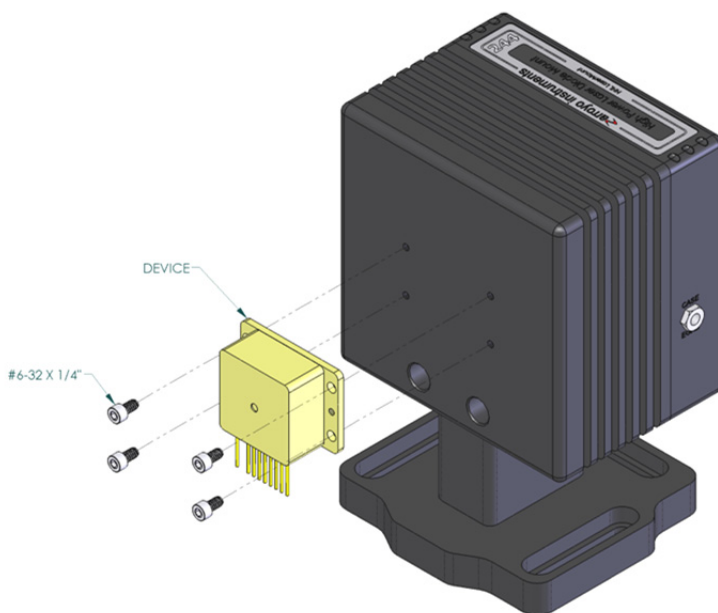

Your fixture is now ready for use. Additional technical information can be found below.

Connector Pin-Outs



244 HHL LaserMount Connectors

DB-9 Pin	Description
1, 2 & 3	No Connection
4 & 5	Laser Cathode
6	Photodiode (PD) Cathode
7	Photodiode (PD) Anode
8 & 9	Laser Anode

Laser DB-9 Connector Pin-Out

DB-15 Pin	Description
1, 2, & 9	TE (+)
3, 4, & 10	TE (-)
5 & 6	No Connection
7	Thermistor
8	Thermistor
11	FAN (+)
12	FAN (-)
13 thru 15	No Connection

TEC DB-15 Connector Pin-Out

HHL Pin	Description
1	TEC (-)
2	No Connection
3	Case
4	Laser Anode (+)
5	Thermistor
6	Thermistor
7	Laser Cathode (-)
8	Photodiode (PD) Anode
9	Photodiode (PD) Cathode
10	TEC (+)

HHL Connector Pin-Out

Connection	Description
Tip	+12VDC (8 to 12VDC)
Sleeve	Fan Ground

12V Fan Connector Pin-Out

Technical Specifications

244 HHL LaserMount

LASER PACKAGE SUPPORTED

Package

HHL

Mounting Holes

6-32 x 4

INPUT CONNECTOR

Laser Diode

DB-9, male

Temperature Controller

DB-15, male

Fan

2.1mm round, 8 to 12VDC

GENERAL


Size without base (H x W x D)
[in(mm)]

4.0 (101.6) x 4.0 (101.6) x 3.5 (76.2)


Mounting holes

Slotted holes for ¼-20 (base)
¼-20 x 2 (for post mount)
M6 (for post mount)

Mechanical Specifications

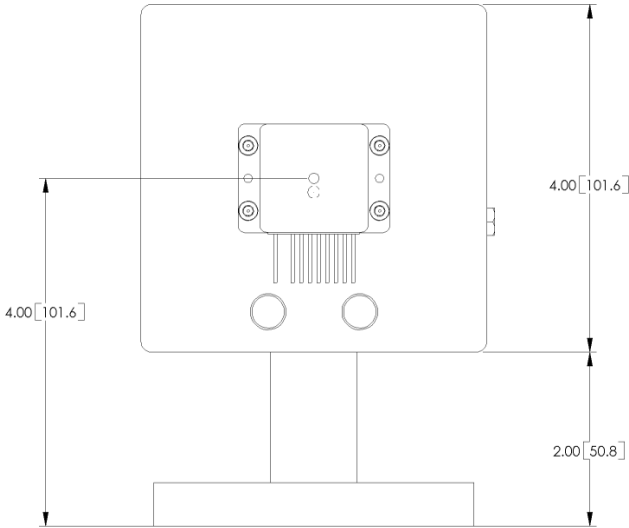

Front View

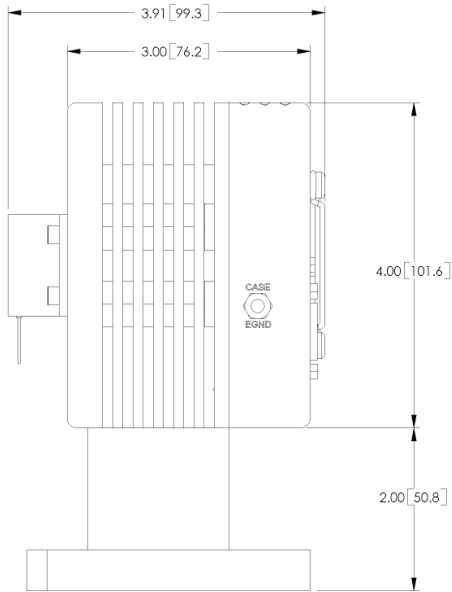

Side View

Laser Diode Protection

Electrostatic discharge and current spikes can be a significant cause of damage to laser diodes, but when proper precautions are taken, these risks can be greatly reduced or eliminated. Arroyo Instruments' controllers offer state-of-art laser diode protection, but no instrument can fully shield the laser from damage. Please take these considerations into account when operating your laser:

1. Always set the current limit at or below the maximum current your laser can handle. This prevents the device from accidentally driving the current too high, either via the set point or from the modulation port. This also provides additional current limiting protection from ESD.
2. Always work in an ESD safe operating environment, including the use of wrist straps, ESD grounded work surfaces and floors, and ESD-safe tools.
3. Where the AC power to the laser driver to temperature controller may be noisy, use isolation transformers or uninterruptible power supplies that provide isolation.
4. Make sure all cables are securely connected and fastening screws are screwed in tight.
5. Do not route power cords or other cables in parallel with the laser or temperature controller cables, as coupling may occur between the cables and inject noise into the laser diode.
6. While it is not possible to create a ground loop through the LaserSource because of it's isolation of all inputs, it is possible when using other equipment. Ensure that any other equipment is properly isolated to avoid any ground loop problems.

Warranty

Arroyo Instruments warrants this product to be free from defects in material and workmanship under normal use and service for a period of one (1) year from date of shipment. It does not apply when the product has been misused, altered or damaged by accident or abnormal conditions of operation. If found to be defective during the warranty period, the product will either be repaired or replaced at Arroyo Instruments's option.

THIS WARRANTY IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESSED OR IMPLIED, INCLUDING IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR ANY PARTICULAR PURPOSE. ARROYO INSTRUMENTS SHALL NOT BE LIABLE FOR ANY INDIRECT, SPECIAL, OR CONSEQUENTIAL DAMAGES RESULTING FROM THE PURCHASE OR USE OF ITS PRODUCTS.

Service and Support

For service and support, contact your local distributor or Arroyo Instruments.

Telephone: +1 (805) 543-1302
Facsimile: +1 (805) 543-1303
Email: support@arroyoinstruments.com
Web: <http://www.arroyoinstruments.com>
Address: 1201 Prospect Street
San Luis Obispo, CA 93401
USA

Notes:



1201 Prospect Street, San Luis Obispo, CA 93401

Tel: (805) 543-1302 Fax: (805) 543-1303

sales@arroyoinstruments.com

www.arroyoinstruments.com